




WEEK TWO SUMMARY

SALIM ROUSTOM


FIXED THE DESKTOP AND INSTALLED ROOT




NORMALIZED THE PMTS

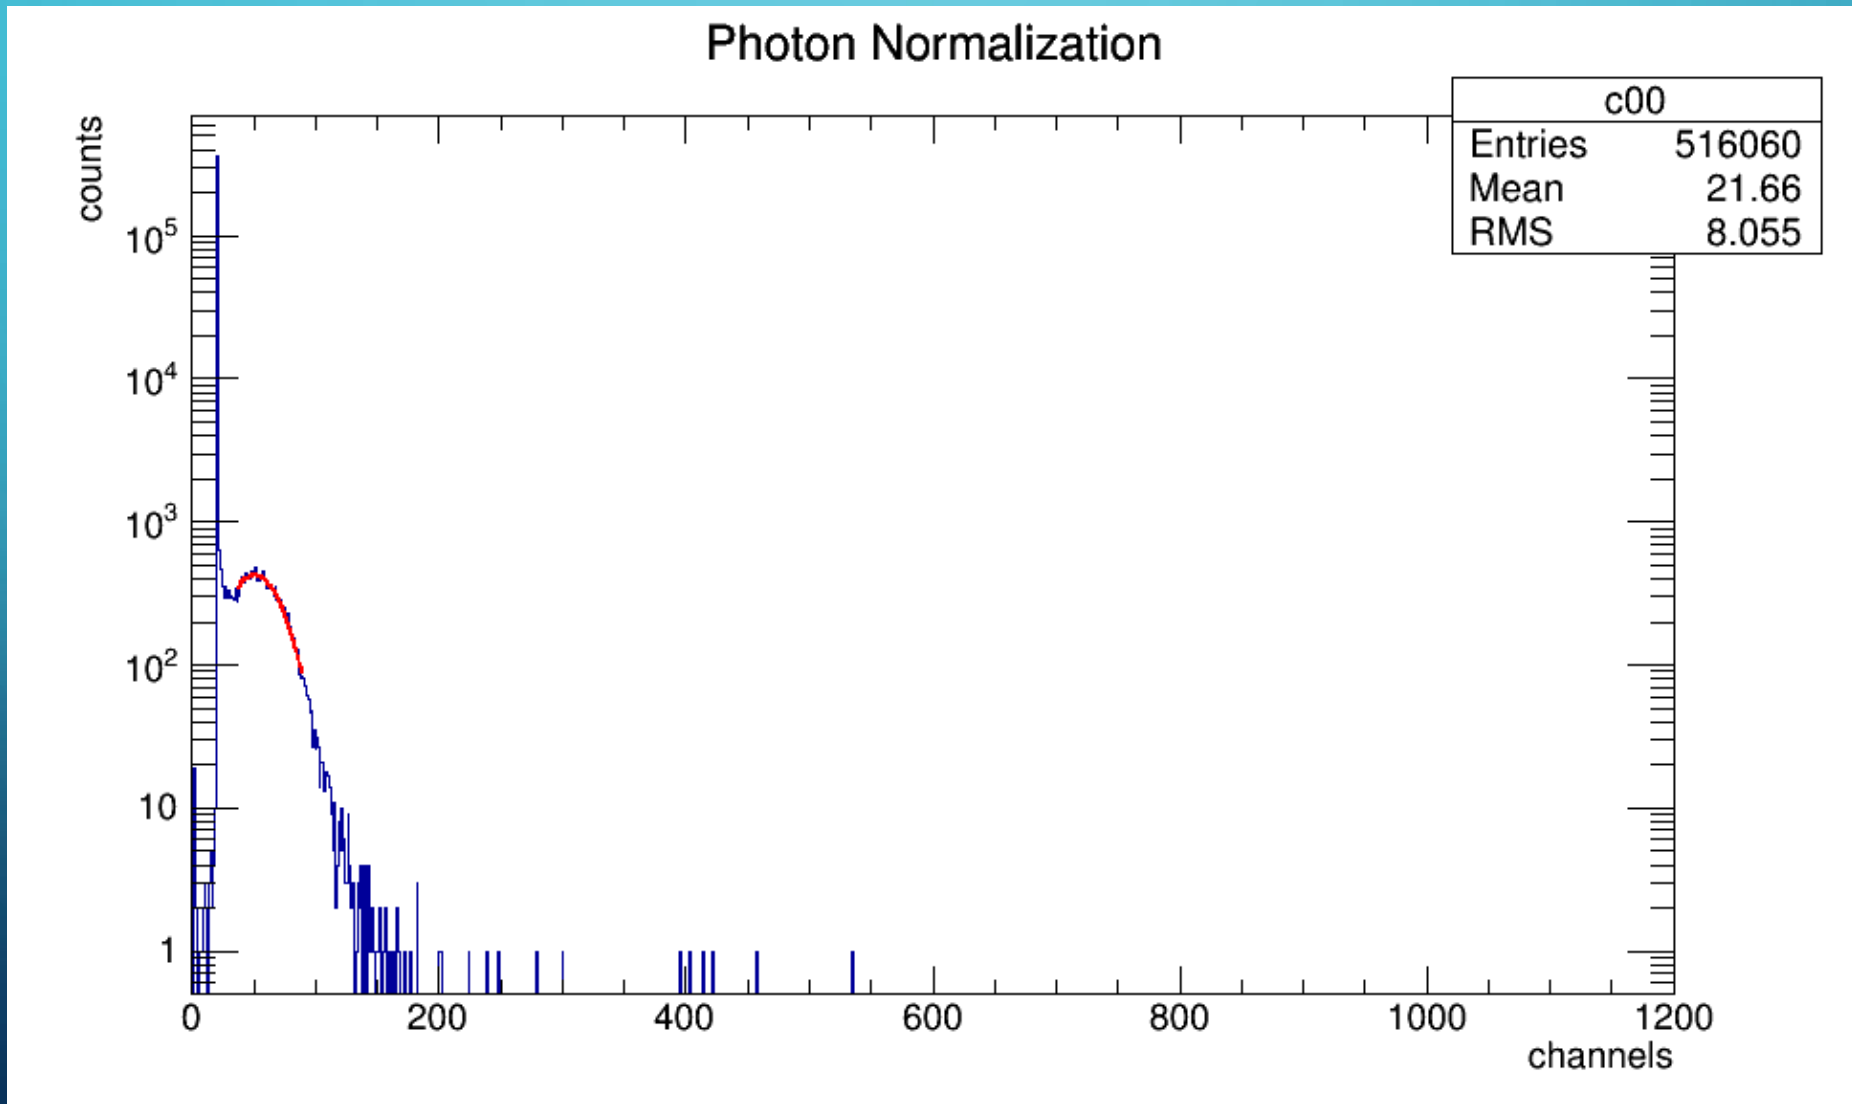

Photon Normalization

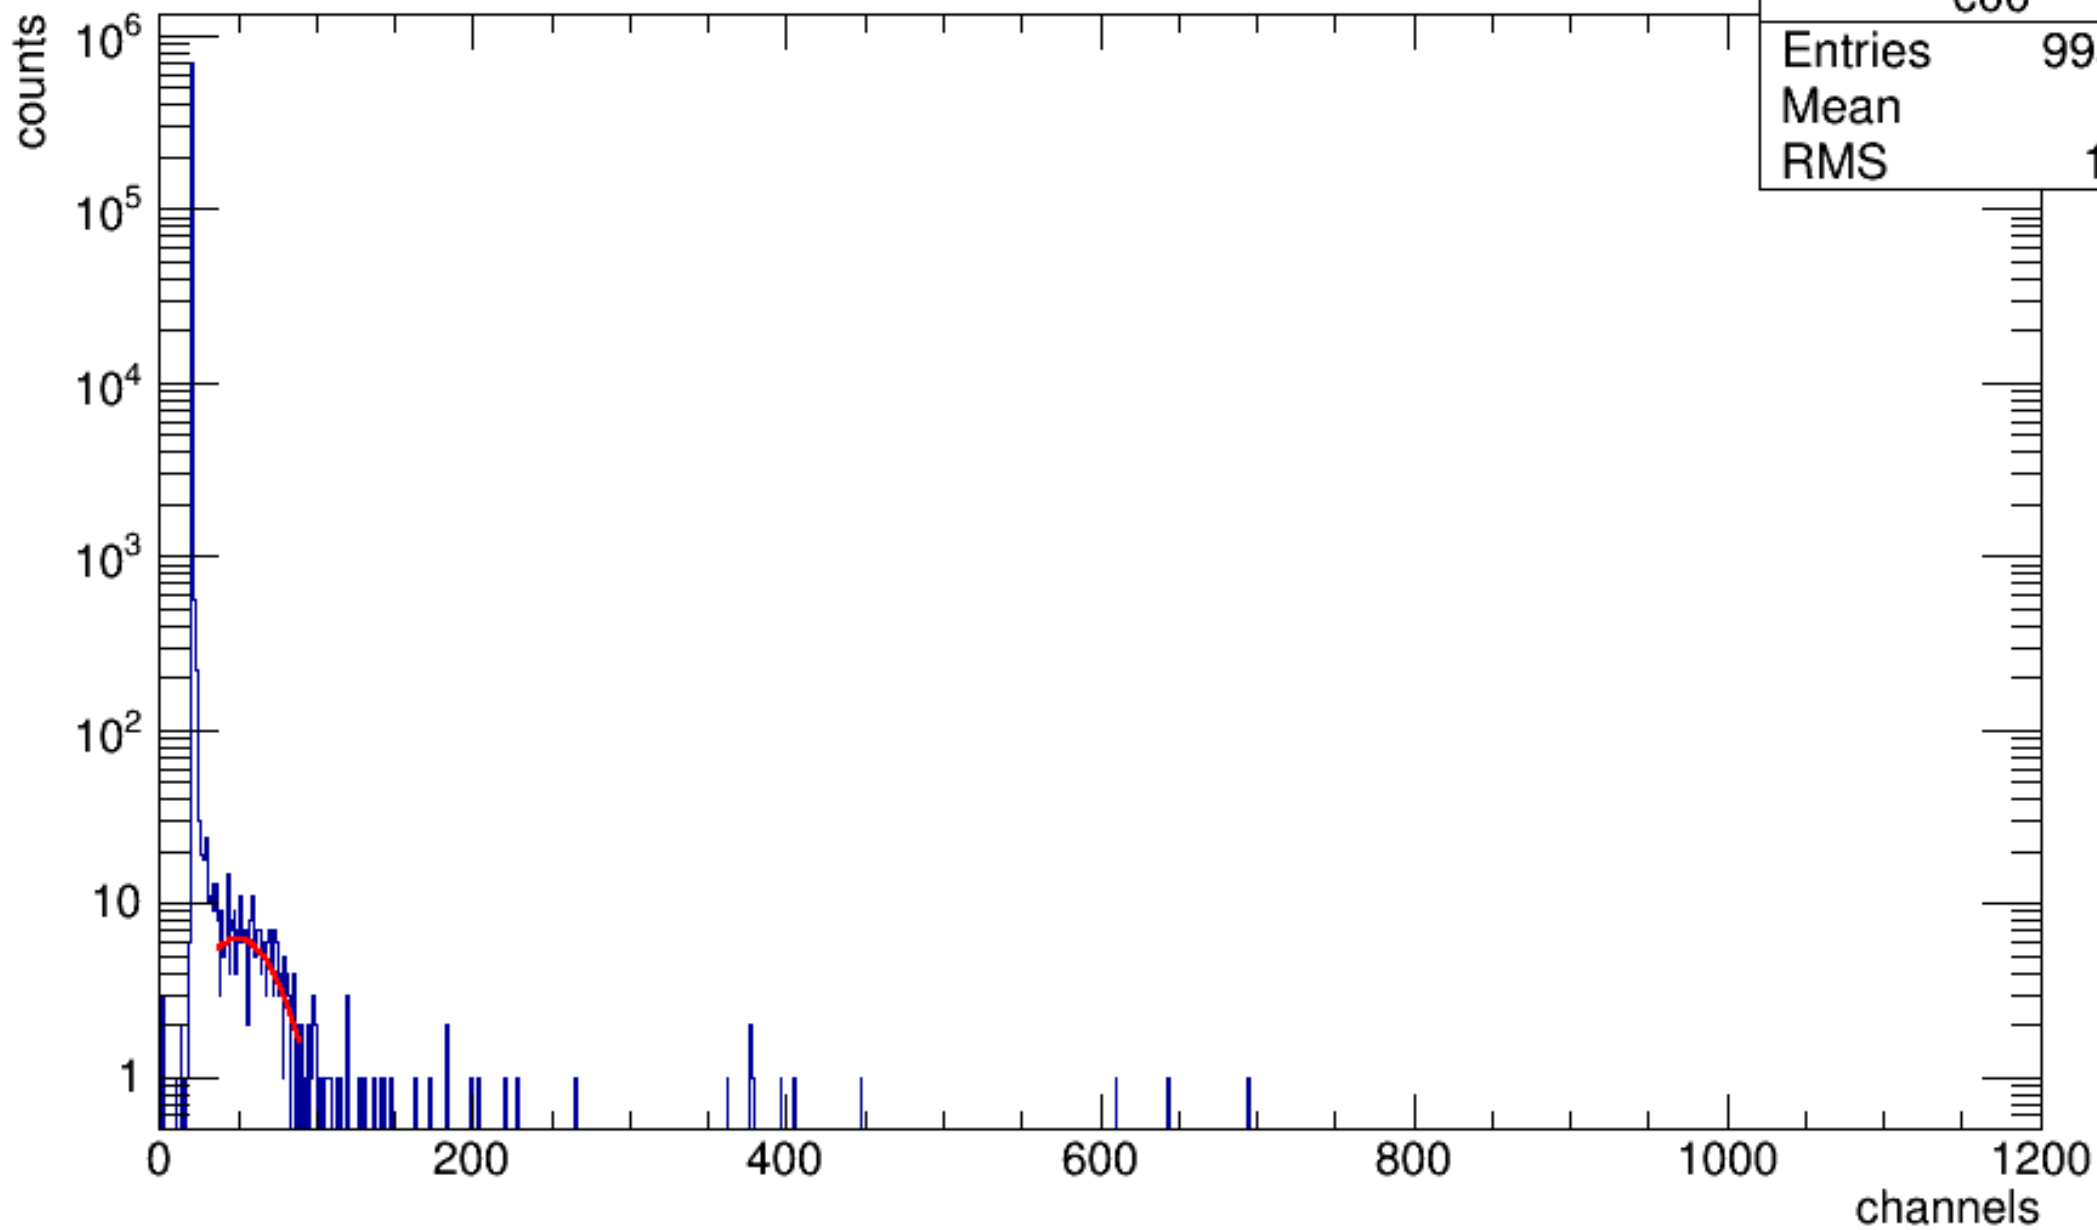


DATA COLLECTION

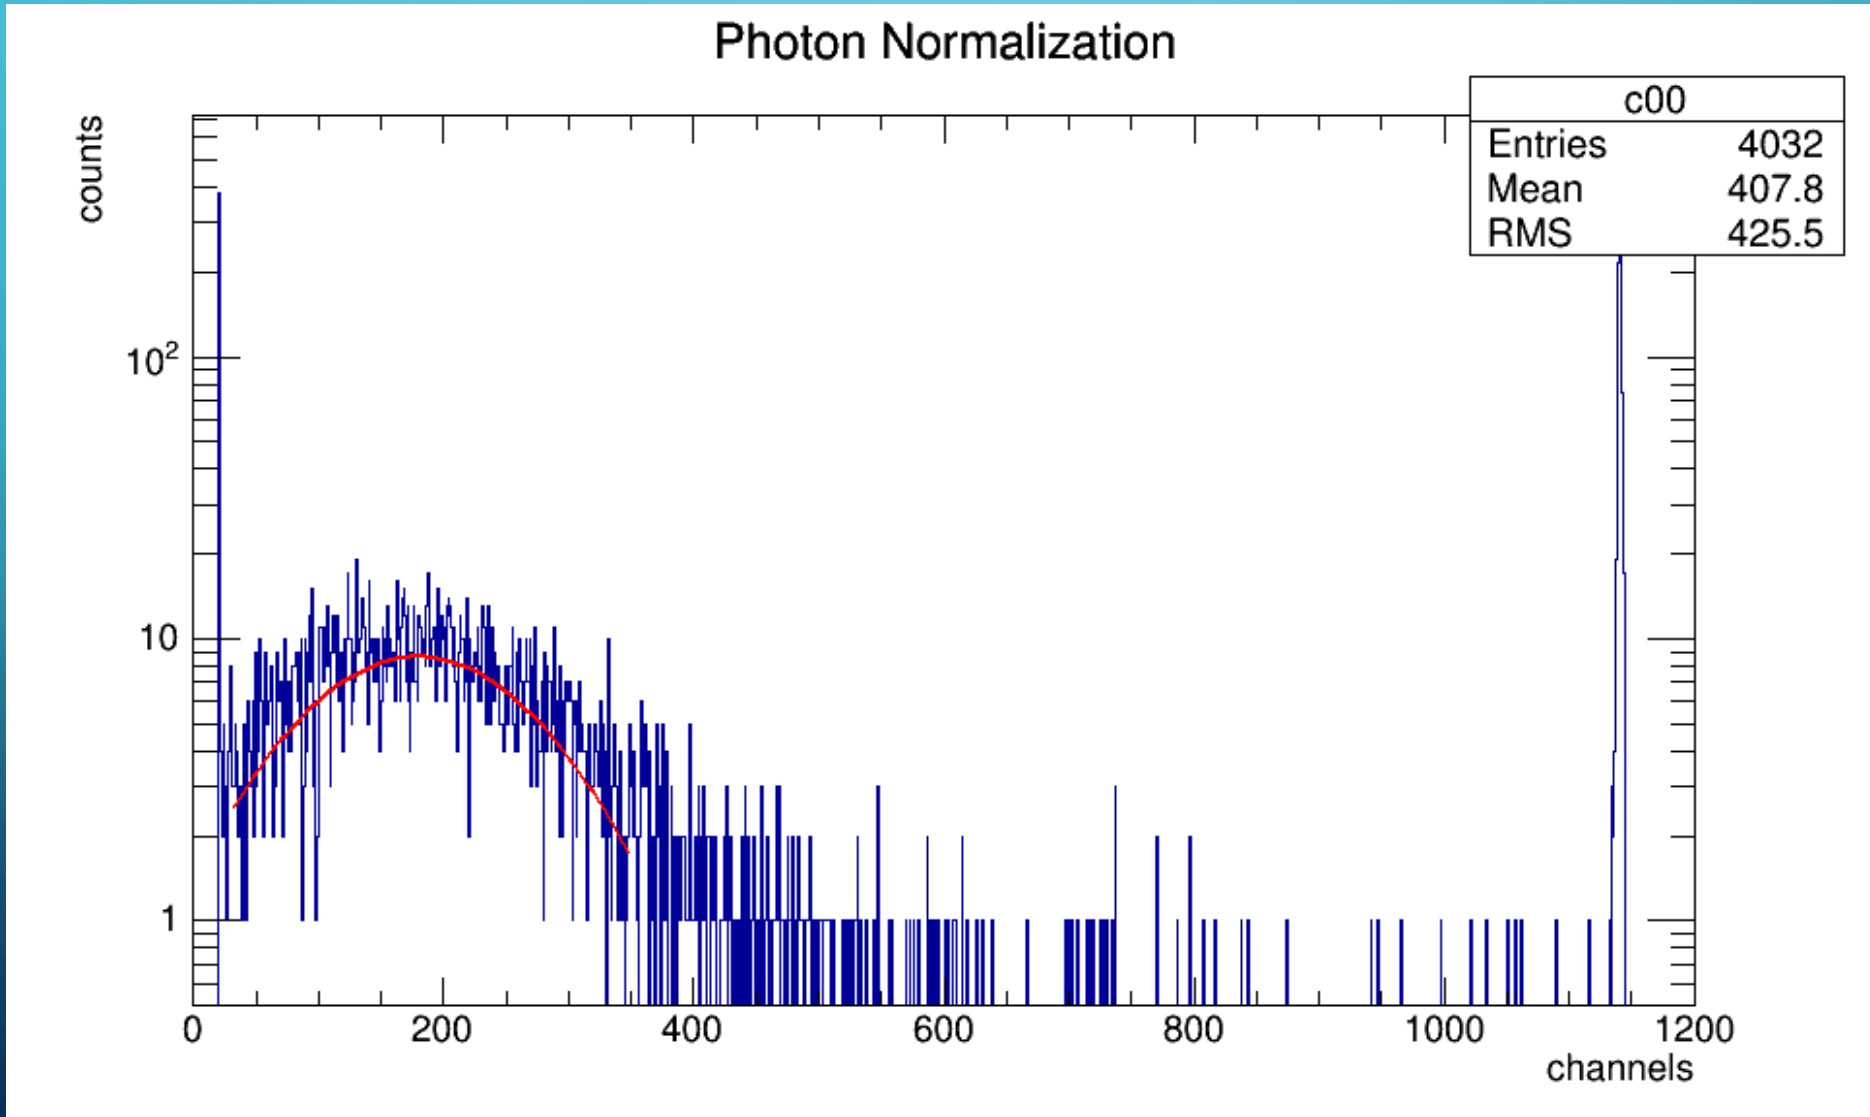


NORMING

Photon Normalization

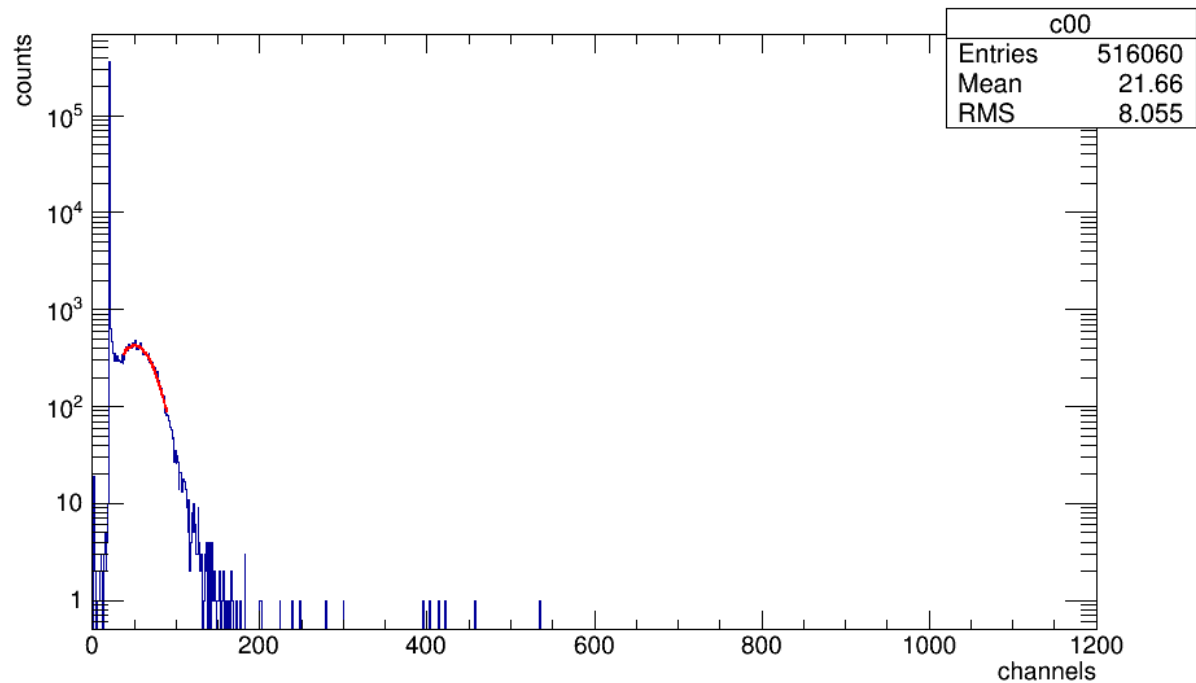

Photon Normalization

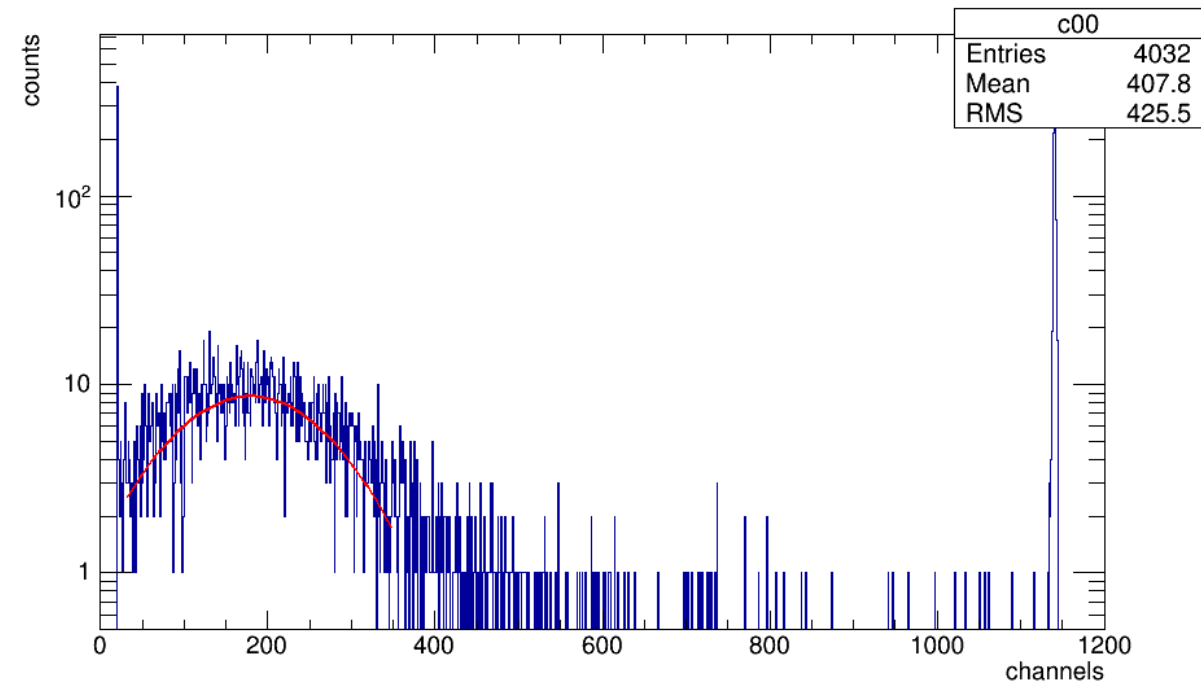

5.393476214586936797643037002552

CONSTANTS

- 10 Tiles of Aerogel
 - SP 30 ($n = 1.03$)
- Aluminized Mylar
- 5" PMT
- 1800 V (1500 V for scintillator PMTs)